

Arboga Elektronikhistoriska Förening

[www.aef.se](http://www.aef.se)

6325




**OWNER'S  
MANUAL**

**REGULATED POWER SUPPLY**

**STABPAC 120**

Serial No .....

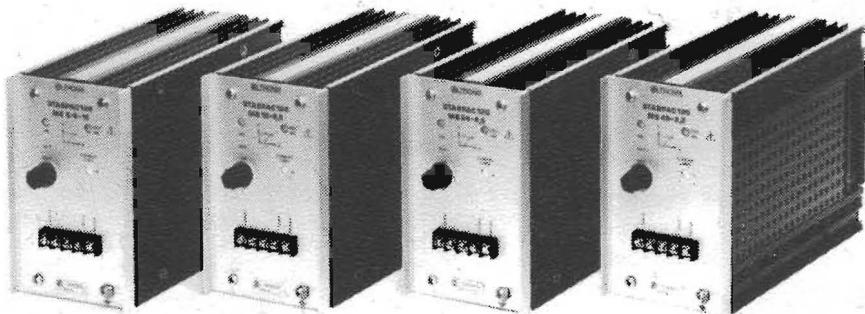RATING DATA <sup>1)</sup>

MODEL	VOLTAGE RANGE $U_{ex}$ (V)	CURRENT $I_{exm}$ (A)	REMARKS
MB 5/6 - 12	4,5 - 5,5 - 6,5	12,0	
MB 12 - 8,5	10,8 - 12,0 - 13,2	8,5	
MB 15 - 6,8	13,5 - 15,0 - 16,5	6,8	
MB 24 - 4,5	21,6 - 24,0 - 26,4	4,5	
MB 28 - 3,8	25,2 - 28,0 - 30,8	3,8	
MB 48 - 2,2	40,0 - 44,0 - 48,0	2,2	

Source voltage  $U_S$   $220V \pm 10\%$ ,  $240V \pm 10\%$  <sup>2)</sup>, 48-63HzAmbient temperature, operating  $t_{amb}$   $0^{\circ}C$  to  $60^{\circ}C$ PERFORMANCE RATINGS <sup>1)</sup> (Data subject to Change)Source current, max  $I_{Sm}$   $0,7A_{rms}$  to  $1,0A_{rms}$ , see Circuit Diagram!Load effect, max (load regulation)  $I_{ex}=0-100\%$   $U_{erL}$   $<5mV$

Source effect (line regulation) $U_{Snom} = U_S \pm 10\%$	$U_{erS}$	<1mV or 0,01%	STABPAC 120 UIL-2(6)
Temperature coefficient $t_{amb} = 0-60^\circ C$	$\alpha$	$<0,01^\circ C^{-1}$	
PARD (ripple and noise) $f_B = 20Hz-20MHz$	$U_{PARD}$	$<0,5mV_{rms}$ or $2mV_{pp}$	
Drift (stability) $\tau = 8h$ , $f_B = 0-20Hz$	$U_{erD}$	0,05%	
Load transient recovery time $I_{ex} = 0-100\%$ Trans. rec.band = $\pm 50mV$	$\tau_R$	<50μs	
Setting range <sup>3)</sup>	$U/I$	$0-1,1 U_{ex\ nom}/0,33-1,05 I_{exm}$	
Remote Resistance Programming	$R_{Pconst}$	$270\Omega/V$	
Voltage Prog.	$U_{const}$	1V/V	
Current Limit region at $U_{ex} = \text{min}$	$I_{CL}$	0,33 to 1,05 $I_{exm}$	
Short Circuit current	$I_{SC}$	0,33 $I_{exm}$	
Reverse current protection max	$I_{Rm}$	12A (model 5/6) 6A (models 12, 15, 24, 28) 3A (model 48)	
Reverse voltage protection max	$U_{Rm}$	1V (One diode forward voltage drop)	
Isolation voltage, max on output terminals relative to the chassis	$U_{isol}$	$\pm 500V$	
Insulating resistance, min ( $U_{test} = 500V$ )	$R_{insul}$	>100MΩ	
Transformer OTP, automatic	$t_{OTP}$	$110^\circ C$	
Storage temperature	$t_{stor}$	$-40^\circ C$ to $85^\circ C$	
Overall dimensions	height width depth	151mm 100mm 246mm	
Mass	m	5,8kg	

- 1) Rating Data and Performance Ratings are expressed in accordance with international recommendations, notably IEC-478.  
 2) Connected for  $U_{Snom} = 240V$  on order or changed at Service Center.  
 3) See Output Chart.

To make the best use of your STABPAC 120, follow these instructions!

STABPAC 120  
UIL-3(6)

#### MAINS (Figure 1)

New units are connected for 220V, 50 Hz mains supply at the factory. The mains cable shall be connected to the three flat tabs ( $2,8 \times 0,5$  mm) at the rear of the unit.

Warning: connect ground tab first and disconnect it last.

Stabpac units have no mains switch and are turned on and off generally with the principal equipment switch.

However an automatic thermal cut-out in the transformer protects the unit against excessive heat. For 220V/240V mains voltage tap-changing, see Service Instruction STP120-1.



Figure 1

#### VOLTAGE ADJUSTMENT (Figure 2)

The output voltage can be set to any value within the nominal range by means of the "VOLT adj"-potentiometer on the front panel.




Figure 2

#### CURRENT LIMIT (Figure 2)

The maximum limiting current "a" on the fold-back curve can be adjusted downwards by the "CURRENT LIMIT a"-potentiometer on the front panel.

#### CURRENT RETURN FUSE (Figure 2)

There is a protective fuse in the minus-lead. If the fuse is blown it should be replaced by a new one carrying the same rating as indicated on the front panel.

#### POWER REGIONS (Figure 3)

The voltage range has two power regions. By changing taps on the transformer, full current can be obtained either in the lower or in the upper voltage range.

Note! The unit can be set to any value within the total specified voltage range in both cases.




Figure 3

STABPAC 120  
UIL-4(6)

To change from the lower range (standard on delivery) to the upper range, remove the two upper screws on the front panel, the upper extrusion and the perforated side covers. Change over the connections on the transformer as indicated in the diagram. Replace the covers and the upper extrusion.

#### OVERTVOLTAGE PROTECTION—OVP (Figure 4 and 5)

Model MB 5/6 has an overvoltage protection as standard, this feature being optional on other models.

The OVP is factory adjusted to 10% or at least 1,5V above the maximum nominal output voltage. This value can be set to within the voltage range by the "adj OVP"-potentiometer on the front panel.

For a voltage exceeding this range, connect an external power supply to the output terminal and limit its output current to 10% of the maximum current of the STABPAC 120. Set the external power supply to the desired voltage. Adjust the "adj OVP"-potentiometer to the limit where it crowbars the external supply. To add OVP on other models, remove the cover lid on the lower extrusion. Introduce a SCR (part no. H502939) in the SCR-socket with the insulator placed underneath the SCR. Tighten the SCR to the chassis with the tapping screws.

#### WARNING!

In the units without OVP-option the "adj OVP"-potentiometer has to be left in the full clockwise position.

#### LOAD CONNECTION (Figure 6)

The output terminals are floating with respect to the chassis and may be used at any level within +500V.

Connect your load to the "+"-and"-"-terminals on the front panel, verify that the sense-links remain in contact with the terminals.

If desireable, compensate against conductor inductance with a capacitor across the load.



Figure 4




Figure 5




Figure 6

## REMOTE SENSING (Figure 7)

Losses in load conductors can be compensated for by using remote sensing. Voltage drops of up to several volts may be accepted by the regulating circuit, but normal practise is to limit them to 0,5V on each load conductor. Remove the sense-links and connect wires from the "+SENSE"- and "-SENSE"-terminals to the load. Twist the wires with the load conductors. Compensating capacitor across the load might be useful.

STABPAC 120  
UIL-5(6)




Figure 7

## REMOTE PROGRAMMING (Figure 8)

### With resistance control:

The unit is externally programmable. The remote resistance programming is  $270\Omega/V$ .

To maintain the specifications of the unit, the resistor programming shall conform to:  $\pm 1\%$ ,  $\pm 50\mu p$  and  $>1/2 W$ .

Adjust the output voltage to its maximum value (the "volt-adj" potentiometer turned fully CW). Remove the "-SENSE"-link and insert the resistor programming between the "PROGR"-terminal and the "-"-terminal, or the negative side on the load when remote sensing is used. Place a  $0.68\mu F$  capacitor in parallel with the resistor to prevent noise and ripple.

### With voltage control:

The Stabpac unit can also be programmed with an externally connected input voltage. The out-put voltage change will maintain a one-to-one ratio with the programming input voltage.

The programming supply must have a reverse current capability of  $4mA$ .

Adjust the output voltage to its minimum value (the "volt-adj" potentiometer turned fully CCW). Remove the "-SENSE"-link and connect the programming supply between the "PROGR"-terminal and the "-"-terminal, or the negative side on the load when remote sensing is used.

Important! The unit is programmable below the nominal range, but the output current is restricted by the foldback curve. It falls towards about  $1/3$  of the maximum current at zero voltage.





Figure 8



## PARALLEL OPERATION OF UNITS

Two or more units can be used in parallel to obtain more current. Due to the "hard-to-set-equal" probability, a slight voltage step occurs as unit after unit feeds current. By Master-Slave operation the current is fed evenly from the units (see Service Instruction STP120-2).

## SERIES OPERATION OF UNITS (Figure 9)

Two or more units may be used in series, up to a maximum sum which depends on the isolation limitation to the chassis of 500V. If any part of the load-line falls outside the combined rating curves let the voltage level to be established before the units are loaded.

STABPAC 120  
UIL-6(6)

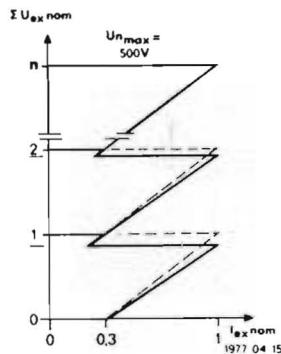


Figure 9

## COMBINATION OF OPERATIONAL MODES

Any form of combination of operational modes is possible, provided each individual instruction is followed.

## MOUNTING (Figure 10)

This unit is designed to be mounted in the upright position, in all cases of normal convection cooling. The unit is provided with fixed M4-nuts on the sides and slots for either M4- or B8-tapping screws. When the slots are used, the screws shall penetrate the slots to at least 12mm for secure fixing. The unit can also be mounted in the STABRAC C, a crate specially designed to house STABPAC-units.



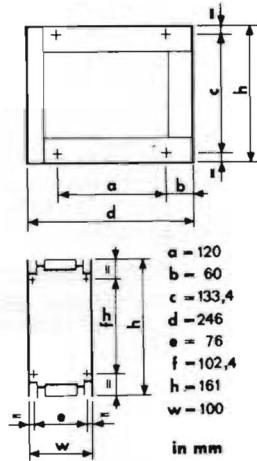


Figure 10

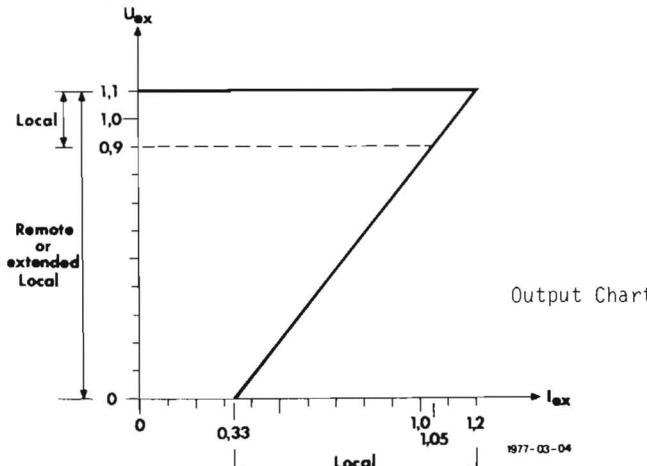


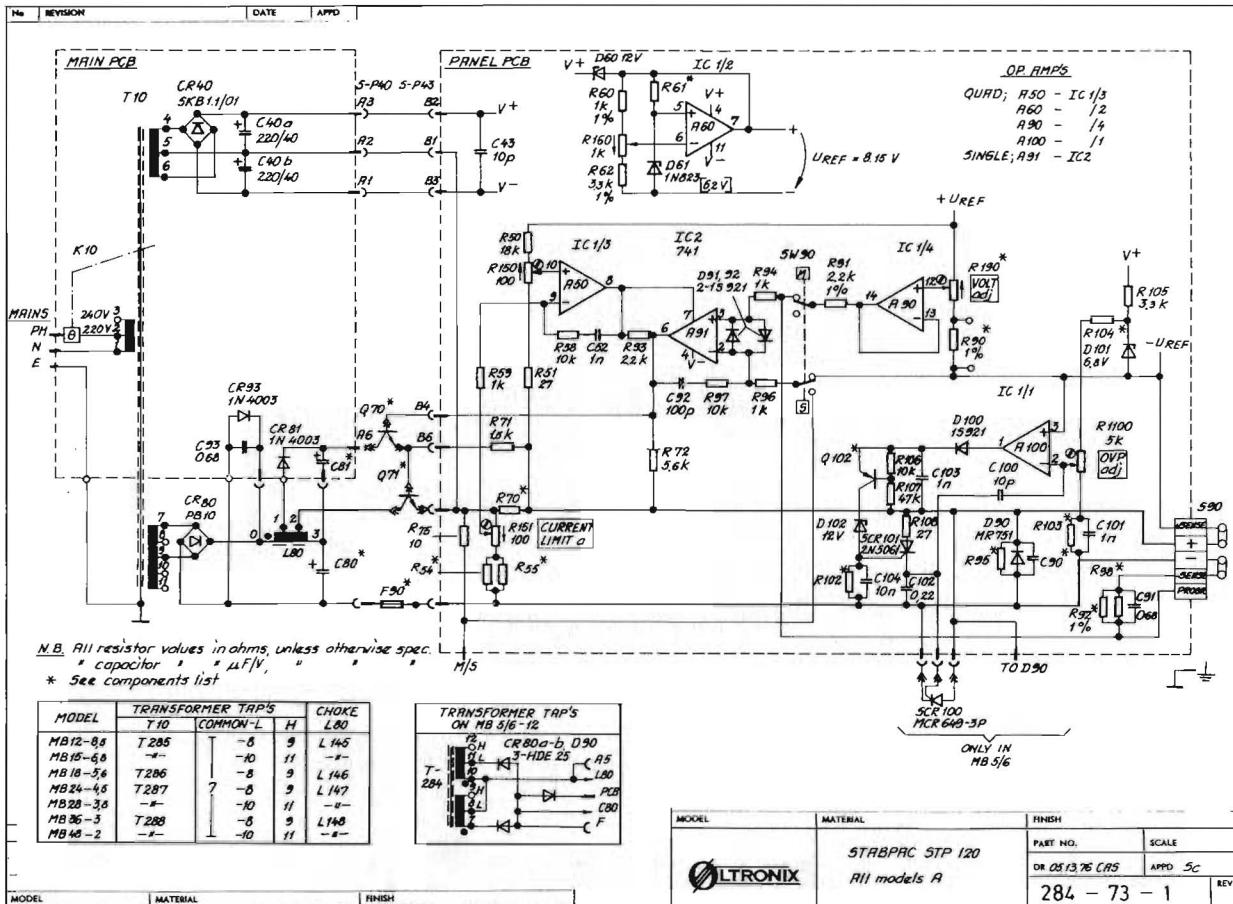

MODEL COMP.	MB5/6-12	MB12-8,5	M815-6,8	MB24-4,5
C80	2-22mF/16V	2-10mF/40V	idem	2-4,7mF/63V
C81	4,7mF/16V	2,2mF/16V	idem	470µF/25V
C90	2-470µF/16V	2-220µF/40V	idem	2-100µF/63V
CR80	2-HDE25-2	PB10	idem	idem
F90	12,5A, fast	10A, fast	8A, fast	5A, fast
L80	L144	L145	idem	L147
O70	2N6290	idem	idem	2N6292
O71	2N3771	idem	idem	2N6254
O102	BC1788	idem	idem	2N5401
R54	5,6k	22k	idem	27k
R55	82k	22k	47k	-
R70	10m	14m	idem	26,5m
R90	18k 1%	20k 1%	idem	idem
R92	1,8k 1%	3,9k 1%	5,6k 1%	8,2k 1%
R95	1k	3,3k	idem	4,7k
R98	-	47k	68k	56k
R102	270	820	idem	1,5k
R103	8,2k	15k	idem	22k
R104	6,8k	idem	idem	5,6k
R190	10k	5k	10k	5k
R1100	5k	idem	idem	idem
T10	T284	T285	idem	T287
SCR100	MCR649-3P	(MCR649-3P)	idem	idem
D90	HDE25-2	MR751	idem	idem

Valid for units with PCB no M10 5336.

PART NO	SCALE
--	--
MTRL NO	--
SURF. TREAT.	--
DRAWN DATE 1977-03-14 SIGN <i>JK</i>	
FREEZE DATE 1977-03-14 SIGN <i>SC</i>	
<input checked="" type="checkbox"/> AB <input type="checkbox"/> BV <input type="checkbox"/> AG <input type="checkbox"/> GmbH	
OLTRONIX	
COMPONENTS LIST	
FAMILY STP120 MODEL all A-vers.	
DRWG NO	
284 — 74 — 1A	

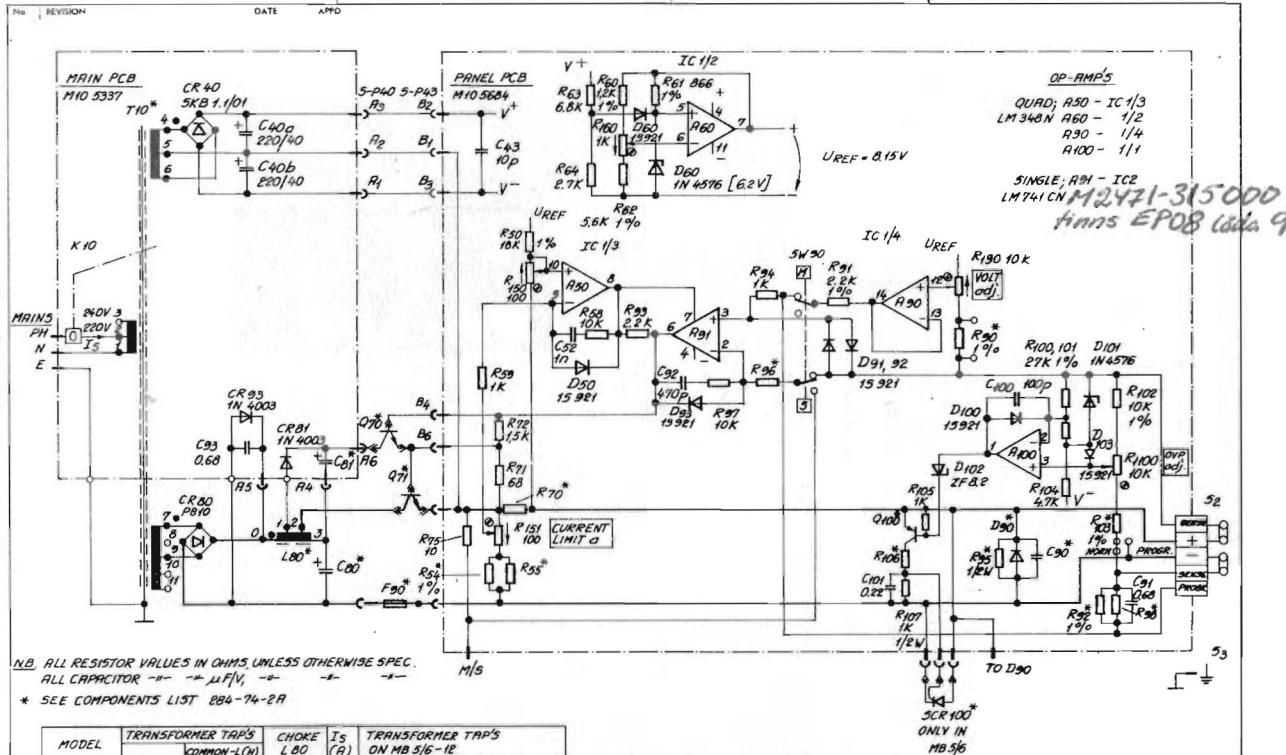

MODEL	TRANSFORMER TAP'S		CHOKES L80	I <sub>S</sub> (A)	TRANSFORMER TAP'S ON MB 5/6-12
	COMMON-L(H)	T-10			
MB5/6-12	T 284	SEE FIGURE	L 144	0.8	2 H CR800-b D90
MB12-8.5	T 285	-8 (T)	L 145	1.05	2 L K3 S-HDE 25-5-C A5
MB15-6.0	-	-	-	-	L80
MB20-4.5	T 287	-8 (9)	L 147	-	PCB
MB20-3.0	-	-	-	-	D90
MB36-3	T 288	-8 (9)	L 148	-	C80
MB48-2	-	-	-	-	-
		-10 (11)	-	-	
		-10 (11)	-	-	

MODEL

MATERIAL

FINISH

MODEL	MATERIAL	FINISH	
		PART NO.	SCALE
STABPAC 120		DR 76.12.06 3G/BB	APPRO 76.12.23.5C

**OLTRONIX**

All models version B

284 - 73 - 2 REV

COMP.	MODEL	MB5/6-12	MB12-8,5	MB15-6,8	MB24-4,5	MB28-3,8	MB48-2,2
C80	2-22mF/16V	2-10mF/40V	idem	2-4,7mF/63V	idem	2-3,3mF/100V	
C81	4,7mF/16V	2,2mF/16V	idem	470μF/25V	idem	220μF/40V	
C90	2-470μF/16V	2-220μF/63V <sup>1)</sup>	idem	2-100μF/63V	idem	220μF/100V	
CR80	2-HDE25-2	PB10	idem	idem	idem	idem	
D90	HDE25-2	MR751	idem	idem	idem	MR501	
F90	12,5A, fast	10A, fast	8A, fast	5A, fast	idem	2,5A, fast	
L80	L144	L145	idem	L147	idem	L148	
Q70	2N6290	idem	idem	2N6292	idem	idem	
Q71	2N3771	idem	idem	2N6254	idem	2N3055/90	
Q100	BC178B	idem	idem	2N5401	idem	idem	
R54	5,36k 1%	13k 1%	16,2k 1%	25,5k 1%	30,1k 1%	51,1k 1%	
R55	-	-	-	-	-	-	
R70	11m	16m	20m	30m	35m	61m	
R90	13,7k 1%	21,5k 1%	22,1k 1%	21,5k 1%	idem	23,2k 1%	
R92	1,87k 1%	3,83k 1%	4,75k 1%	7,68k 1%	8,87k 1%	15k 1%	
R95	120 1/2W	680 1/2W	820 1/2W	4,7k 1/2W	5,6k 1/2W	10k 1/2W	
R98	-	-	-	-	-	-	
R103	5,62k 1%	43,2k 1%	idem	100k 1%	idem	205k 1%	
R106	100	270	idem	560	idem	1,2k	
SCR100	MCR649-3P	(MCR649-3P)	idem	idem	idem	idem	
T10	T284	T285	idem	T287	idem	T288	


<sup>1)</sup> 470μF/40V  
220μF/40V

Valid for units with PCB no M10 5684.



PART NO --	SCALE --			NAME		
MTRL NO --				COMPONENTS LIST		
SURF. TREAT. --		FAMILY STP120 MODEL all B-vers.				
DRAWN DATE 1977-04-04	SIGN	FREEZE DATE 1977-04-04	SIGN	BV	GmbH	DRWG NO 284 — 74 — 2A
<input checked="" type="checkbox"/> AB		<input type="checkbox"/> AG				

MASTER-SLAVE OPERATION

- a) Connect the M/S-output terminal on the Master-unit to the "PROGR"-terminal on the Slave-unit(s).  
The M/S-terminal is a flat-tab on the panel-PCB, accessible behind the lid on the lower profile.
- b) Switch the M/S-switch to the S-position on the Slave-unit(s).  
The switch is situated at half-height on the panel-PCB, and it is accessible through the left perforated side-cover.  
The S-position is towards the inner of the unit.
- c) Remove the "-SENSE"-link on the Slave-unit(s).
- d) Connect parallelwise the "+"-and "-"-terminals to the load.  
Use conductors of equal length.
- e) The "VOLT adj"-potentiometer on the Master-unit will control all of the outputs.

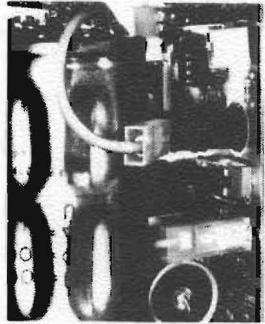


b)

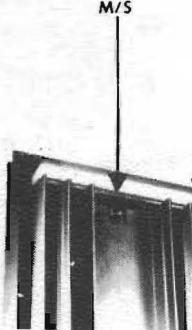

a)

MAINS VOLTAGE TAP-CHANGING

- a) Disconnect the power supply from the mains.
- b) Remove the two upper screws on the front panel and the two fixing screws for the upper extrusion.
- c) Remove the side covers.
- d) Move the soldered wire to the new position as indicated in the figure below.
- e) Assemble the power supply and change on the sticker at the rear the voltage to the new value.

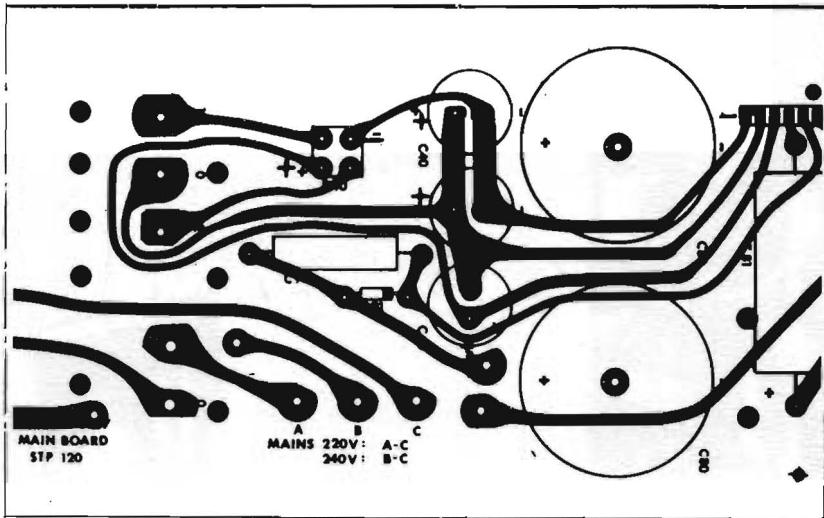



OLTRONIX LABOR AG  
Rüschlistrasse 21  
CH 2502 BIEL  
Switzerland  
Tel: 032/23 8103  
Tlx: 34637

OLTRONIX GMBH  
Postfach 2011  
D 757 BADEN B OOS  
West Germany  
Tel: 07221/616 53  
Tlx: 781110

POWER ELECTRONICS BV  
Euroweg 15  
LEEK (Gr)  
Holland  
Tel: 05945/2700, 2784  
Tlx: 53301

OLTRONIX AB  
Jämtlandsgatan 125  
S-162 29 VÄLLINGBY  
Sweden  
Tel: 08/8703 30  
Tlx: 10738